

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25

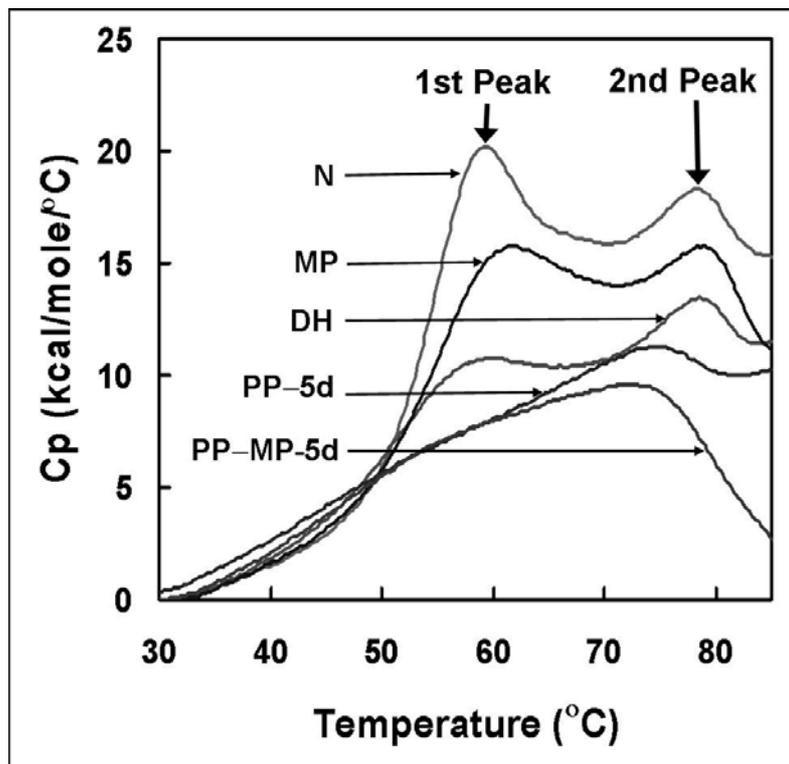


Figure 4—DSC profiles of BSAs. DSC scans were performed with protein solution of 1 g/L in 20 mM phosphate buffer (pH 7.4). These samples were heated in the calorimeter at a scan rate of 1 °C /min over a range of 30–85 °C. For definitions of N, DH, MP, PP, and PP–MP, see Figure 1.

Figure 4.

Enomoto and others.